



**Taha Kimia TajhizCo.**



**Core Lab**




# **PVT Cell 250 ml 1500 bar Full Visibility Datasheet**

**Reservoir Fluid Analysis - PVT / PVT Studies**



## PVT 250/1500 Full Visibility

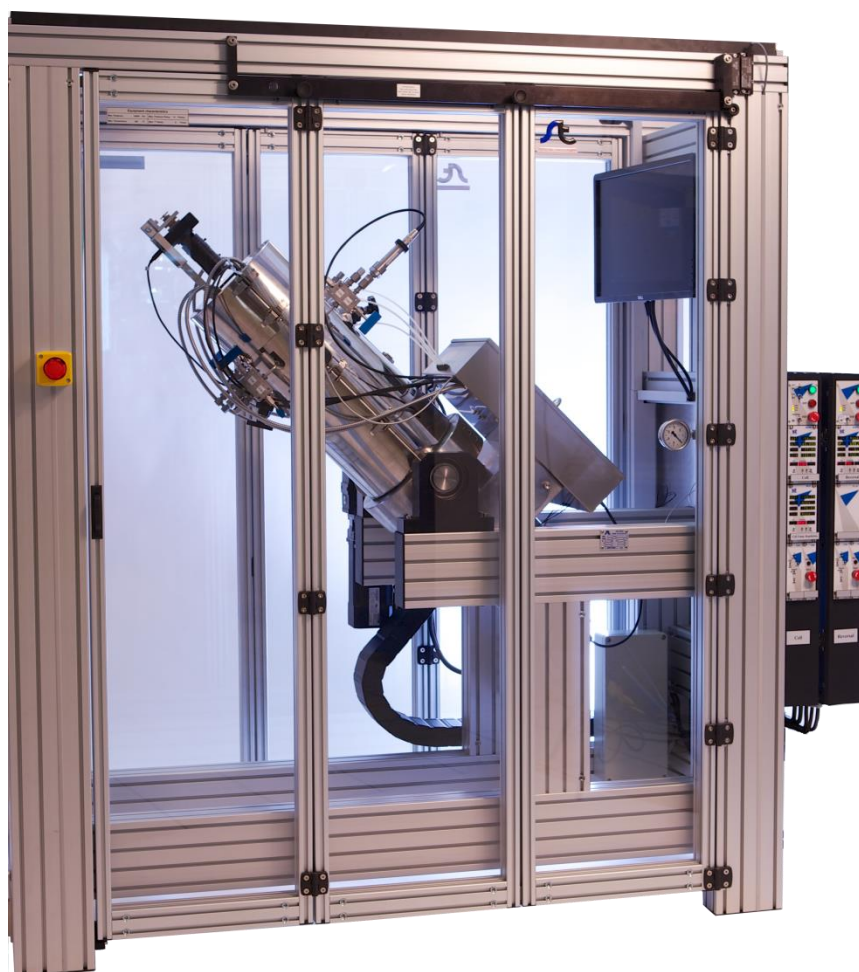

### General Features

Our Reservoir Fluid PVT Analysis System composed of one set of PVT instrument (PVT 250/1500 full visual 250cc) and some ancillary equipment, as gasmeter, HP pressure sample cylinders, viscometer, etc. is able to perform analysis of different GOR reservoir fluids as crude oil, volatile oil, gas condensate and gas under high pressure and temperature conditions.

This system can process the comprehensive evaluation for oil and gas reservoirs.

Specifications	
Max. Working pressure	1500 bar
Max. Working Temperature	Ambient to 200°C
PVT Cell Volume	250 ml
Visual volume	250 ml
Accuracy on measurements:	
Pressure	0.1 bar
Temperature	±0.1°C
Liquid deposit	0.005 ml
Bubble/dew point repeatability	±0.35 bar
Resisting corrosive abilities	CO <sub>2</sub> and H <sub>2</sub> S



## PVT 250/1500 Full Visibility

### Measurements

The PVT 250/1500 with accessories is designed to perform :

- A complete PVT study on oil and volatile oil GOR < 800 Sm<sup>3</sup>/m<sup>3</sup> conducted in 4 stages:
  - Constant Composition Expansion (i.e. CCE) at constant temperature,
  - Differential vaporization at constant temperature,
  - Separation tests (several stages at different temperatures)
  - Viscosity measurement
- A complete PVT study on gas condensate with high GOR conducted in 2 stages:
  - Constant mass depletion (i.e. CMD)
  - Constant volume depletion (i.e. CVD),
- A recombination of separator oil or condensate and separator gas under reservoir conditions
- An analysis of viscosity, density, composition (accessories in option)
- Z factor determination
- Dew point determination by IR
- GOR

### Characteristics

- Constant temperature control system
- Embedded motorized piston displacement pump
- Stirring by magnetic coupling
- Automatic valves
- Control cabinet
- Calibrated pressure sensor and temperature sensor
- CCD digital video camera 6M pixels
- Data acquisition and processing system
- High pressure valves, pipes and filters
- Back pressure regulator CVD valves (option)
- Phase state processing software (option)
- Uninterruptible power supply (option)
- Cooling system for PVT cell -20°C (option)

### Example of synoptic

